

# Rapid and Robust Protein Chromatography

## Chromolith® WP 300 RP-18 2 mm I.D. HPLC Columns

The most hydrophobic of the Chromolith® WP 300 line, the RP-18 column is useful for the resolution of peptides and smaller proteins. One critical quality attribute (CQA) required by regulatory bodies is the peptide map of a biotherapeutic. Peptide maps generated by RP-HPLC provide valuable information about protein structure, stability, and purity. To be effective, the RP-HPLC column must be able to resolve a high percentage of the peptides in the sample. The more peptides, the better the information. The Chromolith® WP 300 RP-18 column gives unsurpassed RP-HPLC resolution of peptide maps from enzymatic digests. The improvements in silica and bonded-phase chemistry incorporated into the Chromolith® WP 300 line improve resolution by increasing efficiency and reducing peak tailing.

### Key Benefits:



- Monolithic skeleton permits high flow rates to maximize throughput
- 300 Å mesopores permit large molecules to enter without fear of size-exclusion effects
- Matrix-loaded samples can be injected onto the column with little to no sample prep.

### Protein Analysis on Chromolith® WP 300 RP-18

For large molecule separations, high efficiency separations are necessary in order to achieve resolution and good peak shape. Moving to sub-2 µm FPP-packed columns or 2.0 µm SPP-packed columns can deliver that desire; however, this comes at the cost of elevated backpressure. Chromolith® WP 300 RP-18, 2 mm I.D. columns provide UHPLC efficiencies, but at nearly 1/10th the backpressure.

### Chromatographic conditions:

<b>Columns:</b>	Chromolith® WP 300 RP-18 100-2 mm (1.52370.0001) SPP, C18, 160 Å, 2.0 µm, 100-2.1 mm FPP, C18, 300 Å, 1.7 µm, 100-2.1 mm
<b>Mobile phase:</b>	A: water (0.1% TFA) B: acetonitrile (0.08% TFA)
<b>Gradient:</b>	4% B to 60% B in 10 minutes
<b>Flow rate:</b>	0.38 mL/min
<b>Detection:</b>	UV, 220 nm
<b>Column temperature:</b>	30 °C
<b>Injection volume:</b>	0.5 µL
<b>Sample:</b>	HPLC Protein Mix 1 mg/mL, water 1) Ribonuclease 2) Cytochrome C 3) Holo-Transferrin 4) Apomyoglobin

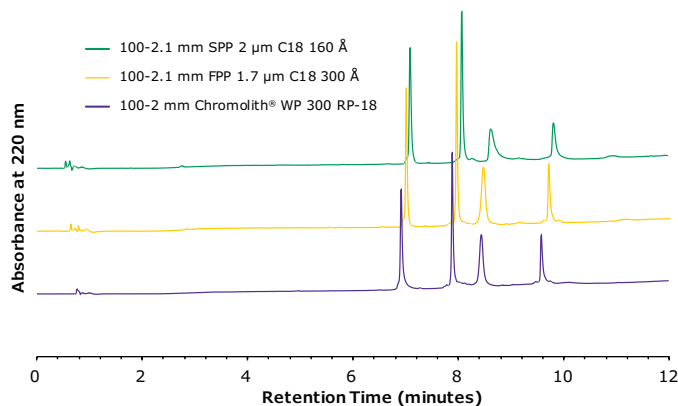


## Excellent Lot-to-Lot Reproducibility

Chromolith® WP 300 RP-18 columns exhibit excellent batch-to-batch reproducibility, as demonstrated below with the same peptide map generated for Cytochrome C using three different Chromolith® WP 300 RP-18 columns across three different batches.

### Chromatographic conditions:

<b>Column</b>	Chromolith® WP 300 RP-18 100-2 mm (1.52370.0001)		
<b>Mobile Phase</b>	A: acetonitrile 0.08% (v/v) TFA B: water 0.1% (v/v) TFA		
<b>Gradient:</b>	<b>Time</b>	<b>%A</b>	<b>%B</b>
	0	5	95
	25.0	30	70
	30.0	30	70
<b>Flow rate:</b>	0.190 mL/min		
<b>Pressure:</b>	18 bar		
<b>Detection:</b>	Vanquish DAD 20 Hz, UV, 214 nm		
<b>Detector cell:</b>	LightPipe 10 mm		
<b>Temperature:</b>	30 °C		
<b>Injection volume:</b>	0.2 µL		
<b>Sample:</b>	Rapid Trypsin Digestion with SOLu-Trypsin Rapid Digestion Kit 2.5 mg Cytochrome C was added in a PCR vial and dissolved in 320 µL Rapid Trypsin Digestion Buffer. In the solution was 80 µL SOLu-Trypsin added and incubated at 60 °C for 1 hour in a Thermomixer. The digestion was quenched by adding 12 µL of hydrochloric acid 32 %.		

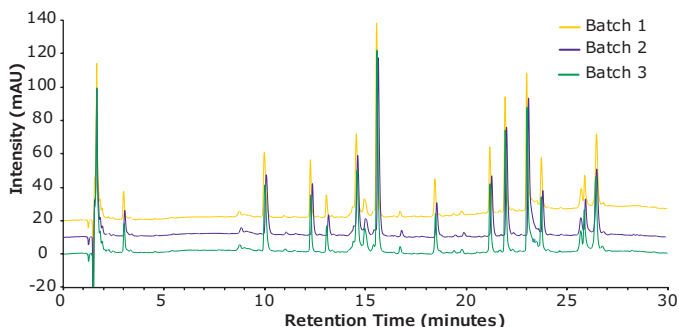


## Antibody Fragment Analysis

Fragment analysis of a monoclonal antibody (mAb), also called middle-up analysis, is a useful technique in characterizing mAb domains without the inherent complexity of a peptide map. High efficiency is needed here to resolve subtle, structural variants of the mAb domains. The Chromolith® WP 300 RP-18 column is able to achieve the same separation efficiency and sensitivity as sub-2 µm FPP and 2.0 µm SPP-packed columns but at only 20% of the backpressure of those columns.

### Chromatographic conditions:

<b>Column</b>	Chromolith® WP 300 RP-18, 2 mm I.D. (1.52370.0001) SPP, C18, 160 Å, 2.0 µm, 100-2.1 mm FPP, C18, 300 Å, 1.7 µm, 100-2.1 mm	
<b>Mobile Phase</b>	A: Water (0.1% (v/v) TFA) B: Acetonitrile (0.08% (v/v) TFA)	
<b>Gradient:</b>	<b>Time (Min)</b>	<b>%B</b>
	0	20
	1	20
	9	45
<b>Flow rate:</b>	380 µL/min	
<b>Detection:</b>	UV, 220 nm	
<b>Temperature:</b>	80 °C	
<b>Injection volume:</b>	1.0 µL	
<b>Sample:</b>	SigmaMAB, 2 mg/mL (SiLu™ Lite Universal Antibody)	
<b>DTT digest:</b>	60 µL of 40 mM Dithiothreitol (DTT) solution was added in a PCR vial, 40 µL mAb was added and incubated at 37 °C for 30 minutes creating light chain (LC) and heavy chain (HC) parts of the antibody.	

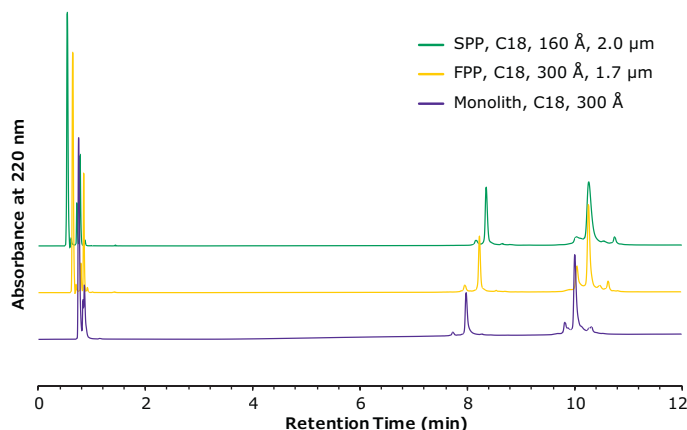

## Ordering Information

Part Number	Description	Length (mm)	I.D. (mm)
1.52370.0001	Chromolith® WP 300 RP-18 Column	100	2
1.52371.0001	Chromolith® WP 300 RP-18 Column	50	2
1.52372.0001	Chromolith® WP 300 RP-18 Guard Columns (3 units)	5	2

## To place an order or receive technical assistance

Order/Customer Service: [SigmaAldrich.com/order](https://www.sigmaaldrich.com/order)  
 Technical Service: [SigmaAldrich.com/techservice](https://www.sigmaaldrich.com/techservice)  
 Safety-related Information: [SigmaAldrich.com/safetycenter](https://www.sigmaaldrich.com/safetycenter)

MilliporeSigma  
 400 Summit Drive  
 Burlington, MA 01803

[SigmaAldrich.com](https://www.sigmaaldrich.com)

