

Important Protocol Change

Standard preparation and concentrations have been updated. Please review before assay setup.

User Guide

MILLIPLEX® Human Cytokine/Chemokine/Growth Factor Panel A Magnetic Bead Panel

96-Well Plate Assay

**HCYTA-60K, HCYTA-60K-PX38
HCYTA-60K-PXBK38, HCYTA-60K-PX48
HCYTA-60K-PXBK48, HCYTPA-76K in HCYTPAB-76SK
HCYTPA-96K in HCYTPAB-96SK**

Introduction	2	Equipment Settings	25
Principle	4	Quality Controls	27
Storage Conditions Upon Receipt	4	Assay Characteristics	28
Reagents Supplied.....	5	Cross-Reactivity	28
Materials Required.....	9	Assay Sensitivities	28
Safety Precautions	9	Precision	30
Symbol Definitions.....	10	Accuracy	32
Technical Guidelines	12	Troubleshooting	33
Sample Collection and Storage	14	Product Ordering.....	36
Preparation of Reagents for Immunoassay.....	16	Analyte Contents of Select Reagents ...	39
Immunoassay Procedure	23	Well Map.....	42
Plate Washing.....	25	Notice	43
		Contact Information.....	43
		Technical Assistance	43
		Standard Warranty	43
		Safety Data Sheets (SDS).....	43

Introduction

"Cytokine" is a general term used for a diverse group of soluble proteins and peptides which act as regulators under both normal and pathological conditions to modulate the functional activities of individual cells and tissues. These proteins also mediate direct interactions between cells and regulate processes taking place in the extracellular environment. Cytokines differ from hormones in that they act on a wider spectrum of target cells. The cytokine group of proteins includes lymphokines, interferons, colony stimulating factors and chemokines. Growth factors are involved in the stimulation of target cell survival, proliferation, differentiation with effects on angiogenesis, vasculogenesis, cell migration, apoptosis, wound healing and embryogenesis.

Cytokine, chemokine and growth factor research plays a significant role in achieving a deeper understanding of the immune system and its multi-faceted response to most antigens, as well as disease states such as inflammatory disease, allergic reactions, IB, sepsis, and cancer.

The MILLIPLEX® portfolio offers the broadest selection of analytes across a wide range of disease states and species. Once the analytes of interest have been identified, you can rely on the quality that we build into each kit to produce results you can trust. In addition to the assay characteristics listed in the protocol, other performance criteria evaluated during the verification process include: cross-reactivity, dilution linearity, kit stability, and sample behavior (for example, detectability and stability).

Each MILLIPLEX® panel and kit includes:

- Quality controls (QCs) to qualify assay performance
- Comparison of standard (calibrator) and QC lots to a reference lot to ensure lot-to-lot consistency
- Optimized serum matrix to mimic native analyte environment in serum and plasma samples
- Detection antibody cocktails designed to yield consistent analyte profiles within panel

In addition, each panel and kit meets stringent manufacturing criteria to ensure batch-to-batch reproducibility. The MILLIPLEX® Human Cytokine/Chemokine/Growth Factor Panel A thus enables you to focus on the therapeutic potential of cytokines and the modulation of cytokine expression. Coupled with the Luminex® xMAP® platform in a magnetic bead format, you receive the advantage of ideal speed and sensitivity, allowing quantitative multiplex detection of dozens of analytes simultaneously, which can dramatically improve productivity.

MILLIPLEX® Human Cytokine/Chemokine/Growth Factor Panel A is part of the most versatile system available for cytokine, chemokine and growth factor research. From our single to multiplex biomarker solutions, we partner with you to design, develop, analytically verify and build the most comprehensive library available for protein detection and quantitation.

MILLIPLEX® products offer you:

- The ability to select a 38-plex or 48-plex premixed kit.
- **Note:** RANTES is provided as a separate bead vial in both premixed bead kits due to different dilution requirements for serum/plasma samples. For more information, please carefully review the "Sample Collection and Storage" section for serum and plasma samples and "Preparation of Reagents for Immunoassay" for preparation of antibody-immobilized beads when assaying RANTES.
- If using tissue/cell culture supernatant samples, the recommended sample dilution is uniform for all analytes. Please review the "Sample Collection and Storage" section for tissue culture supernatant samples.
- The ability to choose any combination of analytes from our panel of 48 analytes to design a custom kit that better meets your needs.
- A convenient "all-in-one" box format that gives you the assurance that you will have all the necessary reagents you need to run your assay.

MILLIPLEX® Human Cytokine/Chemokine/Growth Factor Panel A is a 48-plex kit to be used for the simultaneous quantification of any or all of the following analytes in human tissue/cell lysate and culture supernatant samples and serum or plasma samples: sCD40L, EGF, Eotaxin, FGF-2, FLT-3L, Fractalkine, G-CSF, GM-CSF, GRO α , IFN α 2, IFN γ , IL-1 α , IL-1 β , IL-1RA, IL-2, IL-3, IL-4, IL-5, IL-6, IL-7, IL-8, IL-9, IL-10, IL-12 (p40), IL-12 (p70), IL-13, IL-15, IL-17A, IL-17E/IL-25, IL-17F, IL-18, IL-22, IL-27, IP-10, MCP-1, MCP-3, M-CSF, MDC, MIG, MIP-1 α , MIP-1 β , PDGF-AA, PDGF-AB/BB, RANTES, TGFA, TNFA, TNF β , VEGF-A

For research use only. Not for use in diagnostic procedures.

Please read entire protocol before use.

It is important to use same assay incubation conditions throughout your study.

Principle

MILLIPLEX® products are based on the Luminex® xMAP® technology — one of the fastest growing and most respected multiplex technologies offering applications throughout the life-sciences and capable of performing a variety of bioassays including immunoassays on the surface of fluorescent-coded magnetic beads known as MagPlex®-C microspheres.

- Luminex® products use proprietary techniques to internally color-code microspheres with two fluorescent dyes. Through precise concentrations of these dyes, distinctly colored bead sets of 500-5.6 μm polystyrene microspheres or 80-6.45 μm magnetic microspheres can be created, each of which is coated with a specific capture antibody.
- After an analyte from a test sample is captured by the bead, a biotinylated detection antibody is introduced.
- The reaction mixture is then incubated with Streptavidin-PE conjugate, the reporter molecule, to complete the reaction on the surface of each microsphere.
- The following Luminex® instruments can be used to acquire and analyze data using two detection methods:
- The Luminex® analyzers, Luminex® 200™, FLEXMAP 3D®, and xMAP® INTELLIFLEX, are flow cytometry-based instruments that integrate key xMAP® detection components, such as lasers, optics, advanced fluidics and high-speed digital signal processors.
- The Luminex® analyzer MAGPIX®, a CCD-based instrument that integrates key xMAP® capture and detection components with the speed and efficiency of magnetic beads.
- Each individual microsphere is identified and the result of its bioassay is quantified based on fluorescent reporter signals. We combine the streamlined data acquisition power of Luminex® xPONENT® acquisition software with sophisticated analysis capabilities of MILLIPLEX® Analyst, integrating data acquisition and analysis seamlessly with all Luminex® instruments.

The capability of adding multiple conjugated beads to each sample results in the ability to obtain multiple results from each sample. Open-architecture xMAP® technology enables multiplexing of many types of bioassays reducing time, labor and costs over traditional methods.

Storage Conditions Upon Receipt

- Recommended storage for kit components is 2–8 °C.
- For long-term storage, freeze reconstituted standards and controls at ≤ -20 °C. Avoid multiple (> 2) freeze/thaw cycles.
- **DO NOT FREEZE** Antibody-Immobilized Beads, Detection Antibody, and Streptavidin-Phycoerythrin.

Reagents Supplied

Reagents	Volume	Quantity	Cat. No.
Human Cytokine/Chemokine/Growth Factor Panel A Standard*	Lyophilized	1 vial	HCYTA-8060-1 (for configurable 27-plex) or HCYTA-8060-2 (for 38-plex and 48-plex)
Human Cytokine/Chemokine/Growth Factor Panel A Quality Controls 1 and 2*	Lyophilized	1 vial each	HCYTA-6060-1 (for configurable 27-plex) or HCYTA-6060-2 (for 38-plex and 48-plex)
Human Cytokine Panel A Serum Matrix*	Lyophilized	1	MXHSM-A
Set of one 96-Well Plate with 2 sealers	-	1 set	-
Assay Buffer	30 mL	1 bottle	L-AB
10X Wash Buffer	60 mL	1 bottle	L-WB
Human Cytokine/Chemokine/Growth Factor Panel A Detection Antibodies*	3.2 mL	1 bottle	HCYTA-1060-1 (for configurable 27-plex) or HCYTA-1060-2 (for 38-plex and 48-plex)
Streptavidin-Phycoerythrin*	3.2 mL	1 bottle	L-SAPE3 (Use with Cat. No. HCTYA-1060-1) or L-SAPE10 (Use with Cat. No. HCYTA-1060-2)
Bead Diluent (not provided with premixed bead)	3.5 mL	1 bottle	LBD
Mixing Bottle (not provided with premixed panel)	-	1 bottle	-

* Contains 0.08% Sodium azide

*** For details on which reagents ship with which analytes, see table in "Replacement Reagents" section.

For research use only. Not for use in diagnostic procedures.

Human Cytokine/Chemokine/Growth Factor Panel A Antibody-Immobilized Premixed Magnetic Beads:

Reagents	Volume	Quantity	Cat. No.
Premixed 37-Plex Beads*	3.5 mL	1 bottle	HCYTAPX37-MG
Premixed 47-Plex Beads*	3.5 mL	1 bottle	HCYTAPX47-MG

***Note:** RANTES is provided as a separate bead vial in both premixed bead kits due to different dilution requirements for serum/plasma samples. RANTES can only be added in the premix for samples other than serum/plasma. If measuring RANTES in serum/plasma, it is recommended to use a singleplex kit including RANTES only. For more information, please carefully review the sample preparation for serum and plasma samples and the preparation of antibody-immobilized beads sections below when assaying RANTES.

Included Human Cytokine/Chemokine/Growth Factor Panel A Antibody-Immobilized Beads are dependent on customizable selection of analytes within the panel.

Human Cytokine/Chemokine/Growth Factor Panel A Antibody-Immobilized Magnetic Beads:

Bead/Analyte Name	Luminex® Magnetic Bead Region	Customizable 48 Analytes (50X concentration, 90 µL)		37-Plex Magnetic Premixed Beads	47-Plex Magnetic Premixed Beads
		Available	Cat. No.		
Anti-Human sCD40L Bead	12	✓	HCD40L-MG		✓
Anti-Human EGF Bead	13	✓	HEGF-MG	✓	✓
Anti-Human Eotaxin Bead	14	✓	HETXN-MG	✓	✓
Anti-Human FGF-2 Bead	15	✓	HFGF2-MG		✓
Anti-Human FLT-3L Bead	18	✓	HFLT3L-MG		✓
Anti-Human Fractalkine Bead	19	✓	HFRACKALKN-MG		✓
Anti-Human G-CSF Bead	20	✓	HGCSF-MG	✓	✓
Anti-Human GM-CSF Bead	21	✓	HGMCSF-MG	✓	✓
Anti-Human GROα Bead	22	✓	HGR0-MG		✓
Anti-Human IFNα2 Bead	25	✓	HIFNA2-MG	✓	✓
Anti-Human IFNγ Bead	26	✓	HIFNG-MG	✓	✓
Anti-Human IL-1α Bead	27	✓	HIL1A-MG	✓	✓
Anti-Human IL-1β Bead	28	✓	HIL1B-MG	✓	✓
Anti-Human IL-1RA Bead	29	✓	HIL1RA-MG	✓	✓
Anti-Human IL-2 Bead	30	✓	HIL2-MG	✓	✓
Anti-Human IL-3 Bead	33	✓	HIL3-MG	✓	✓
Anti-Human IL-4 Bead	34	✓	HIL4-MG	✓	✓
Anti-Human IL-5 Bead	35	✓	HIL5-MG	✓	✓
Anti-Human IL-6 Bead	36	✓	HIL6-MG	✓	✓
Anti-Human IL-7 Bead	37	✓	HIL7-MG	✓	✓
Anti-Human IL-8 Bead	38	✓	HIL8-MG	✓	✓
Anti-Human IL-9 Bead	39	✓	HIL9-MG		✓
Anti-Human IL-10 Bead	42	✓	HIL10-MG	✓	✓
Anti-Human IL-12 (p40) Bead	43	✓	HIL12P40-MG	✓	✓
Anti-Human IL-12 (p70) Bead	44	✓	HIL12P70-MG	✓	✓

For research use only. Not for use in diagnostic procedures.

Bead/Analyte Name	Luminex® Magnetic Bead Region	Customizable 48 Analytes (50X concentration, 90 µL)		37-Plex Magnetic Premixed Beads	47-Plex Magnetic Premixed Beads
		Available	Cat. No.		
Anti-Human IL-13 Bead	46	✓	HIL13-MG	✓	✓
Anti-Human IL-15 Bead	47	✓	HIL15-MG	✓	✓
Anti-Human IL-17A Bead	48	✓	HIL17A-MG	✓	✓
Anti-Human IL-17E/ IL-25 Bead	51	✓	HIL17E-MG	✓	✓
Anti-Human IL-17F Bead	53	✓	HIL17F-MG	✓	✓
Anti-Human IL-18 Bead	54	✓	HIL18-MG	✓	✓
Anti-Human IL-22 Bead	55	✓	HIL22-MG	✓	✓
Anti-Human IL-27 Bead	56	✓	HIL27-MG		✓
Anti-Human IP-10 Bead	57	✓	HIP10-MG	✓	✓
Anti-Human MCP-1 Bead	61	✓	HMCP1-MG	✓	✓
Anti-Human MCP-3 Bead	62	✓	HMCP3-MG		✓
Anti-Human M-CSF Bead	63	✓	HMCSF-MG	✓	✓
Anti-Human MDC Bead	64	✓	HMDC-MG		✓
Anti-Human MIG/CXCL9 Bead	65	✓	HMIG-MG	✓	✓
Anti-Human MIP-1α Bead	66	✓	HMIP1A-MG	✓	✓
Anti-Human MIP-1β Bead	67	✓	HMIP1B-MG	✓	✓
Anti-Human PDGF-AA Bead	72	✓	HPDGFAA-MG	✓	✓
Anti-Human PDGF-AB/BB Bead	73	✓	HPDGFB-B-MG	✓	✓
Anti-Human RANTES Bead*	74	✓	HRANTES-MG	*	*
Anti-Human TGFα Bead	75	✓	HTGFA-MG		✓
Anti-Human TNFα Bead	76	✓	HTNFA-MG	✓	✓
Anti-Human TNFβ Bead	77	✓	HTNFB-MG	✓	✓
Anti-Human VEGF-A Bead	78	✓	HVEGFA-MG	✓	✓

***Note:** RANTES is provided as a separate bead vial in both premixed bead kits due to different dilution requirements for serum/plasma samples. For more information, please carefully review the sample preparation for serum and plasma samples and the preparation of antibody-immobilized beads sections below when assaying RANTES.

Materials Required (Not included)

Reagents

- MAGPIX® Drive Fluid PLUS (Cat. No. 40-50030), xMAP® Sheath Fluid PLUS (Cat. No. 40-50021), or xMAP® Sheath Concentrate PLUS (Cat. No. 40-50023)

Instrumentation/Materials







- Adjustable pipettes with tips capable of delivering 25 µL to 1000 µL
- Multichannel pipettes capable of delivering 5 µL to 50 µL or 25 µL to 200 µL
- Reagent reservoirs
- Polypropylene microfuge tubes
- Rubber bands
- Aluminum foil
- Absorbent pads
- Laboratory vortex mixer
- Branson Ultrasonic Cleaner Model No. B200 or equivalent
- Titer plate shaker (VWR® Microplate Shaker Cat. No. 12620-926 or equivalent)
- Luminex® 200™, HTS, FLEXMAP 3D®, MAGPIX® instrument with xPONENT® software, or xMAP® INTELLIFLEX instrument with INTELLIFLEX software by Luminex® Corporation
- Automatic Plate Washer for magnetic beads (BioTek® 405 LS and 405 TS, Cat. No. 40-094, 40-095, Cat. No. 40-096, 40-097 or equivalent) or Handheld Magnetic Separation Block (Cat. No. 40-285 or equivalent)

Note: If a plate washer or handheld magnetic separation block for magnetic beads is not available, one can use a microtiter filter plate (Cat. No. MX-PLATE) to run the assay using a vacuum filtration unit (Vacuum Manifold, Cat. No. MSVMHTS00 or equivalent with Vacuum Pump, Cat. No. WP6111560 or equivalent). If using a filter plate, contact Technical Support for questions.






Safety Precautions

- All blood components and biological materials should be handled as potentially hazardous. Follow universal precautions as established by the Centers for Disease Control and Prevention and by the Occupational Safety and Health Administration when handling and disposing of infectious agents.
- Sodium azide has been added to some reagents as a preservative. Although the concentrations are low, Sodium azide may react with lead and copper plumbing to form highly explosive metal azides. Dispose of unused contents and waste in accordance with international, federal, state, and local regulations.

Symbol Definitions

Ingredient	Cat. No.	Label	
Streptavidin-Phycoerythrin	L-SAPE10		Warning. Causes serious eye irritation. IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.
Streptavidin-Phycoerythrin	L-SAPE3		Warning. Causes serious eye irritation. IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.
10X Wash Buffer	L-WB		Warning. May cause an allergic skin reaction. Wear protective gloves. IF ON SKIN: Wash with plenty of soap and water.
Human Cytokine/Chemokine Panel A Serum Matrix	MXHSM-A	no symbol required	Harmful to aquatic life with long lasting effects. Avoid release to the environment.
Human Cytokine/Chemokine Panel A Standard 1/Human Cytokine/Chemokine Panel A Standard 2	HCYTA-8060-1 HCYTA-8060-2	  	Danger. Harmful if swallowed or if inhaled. Toxic in contact with skin. Causes serious eye damage. May cause damage to organs (brain) through prolonged or repeated exposure. Do not breathe dust/fume/gas/mist/vapours/spray. Wash skin thoroughly after handling. Do not eat, drink or smoke when using this product. Use only outdoors or in a well-ventilated area. Wear protective gloves/eye protection/face protection. IF SWALLOWED: Call a POISON CENTER/doctor if you feel unwell. IF ON SKIN: Wash with plenty of soap and water. IF INHALED: Remove person to fresh air and keep comfortable for breathing. IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing. Immediately call a POISON CENTER/doctor. Specific measures (see supplemental first aid instructions on this label). Store locked up. Dispose of contents/container to an approved waste disposal plant.

For research use only. Not for use in diagnostic procedures.

Ingredient	Cat. No.	Label
Human Cytokine/Chemokine Panel A QC1 & QC2 for Std1/Human Cytokine/Chemokine Panel A QC1 & QC2 for Std2	HCYTA-6060-1 HCYTA-6060-2	<p>Danger. Harmful if swallowed or if inhaled. Toxic in contact with skin. Causes serious eye damage. May cause damage to organs (brain) through prolonged or repeated exposure. Do not breathe dust/fume/gas/mist/vapours/spray. Wash skin thoroughly after handling. Do not eat, drink or smoke when using this product. Use only outdoors or in a well-ventilated area. Wear protective gloves/eye protection/ face protection.</p> <p> IF SWALLOWED: Call a POISON CENTER/doctor if you feel unwell. IF ON SKIN: Wash with plenty of soap and water. IF INHALED: Remove person to fresh air and keep comfortable for breathing. IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing. Immediately call a POISON CENTER/doctor. Specific measures (see supplemental first aid instructions on this label). Store locked up. Dispose of contents/</p> <p></p> <p></p>
Human Cytokine/Chemokine Panel A Detection Antibodies 1	HCYTA-1060-1	<p>Warning. Causes serious eye irritation. IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.</p> <p></p>
Human Cytokine/Chemokine Panel A Detection Antibodies 2	HCYTA-1060-2	<p>Warning. Causes serious eye irritation. IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.</p> <p></p>

Technical Guidelines

To obtain reliable and reproducible results, the operator should carefully read this entire manual and fully understand all aspects of each assay step before running the assay. The following notes should be reviewed and understood before the assay is set up.

- FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.
- Do not use beyond the expiration date on the label.
- Do not mix or substitute reagents with those from other lots or sources.
- The Antibody-Immobilized Beads are light sensitive and must be protected from light at all times. Cover the assay plate containing beads with opaque plate lid or aluminum foil during all incubation steps.
- It is important to allow all reagents to warm to room temperature (20-25 °C) before use in the assay.
- Incomplete washing can adversely affect the assay outcome. All washing must be performed with the Wash Buffer provided.
- The standards prepared by serial dilution must be used within 1 hour of preparation. Discard any unused standards except the standard stock which may be stored at ≤ -20 °C for 1 month and at ≤ -80 °C for greater than one month.
- If samples fall outside the dynamic range of the assay, further dilute the samples with the appropriate diluent and repeat the assay.
- Any unused mixed Antibody-Immobilized Beads may be stored in the Mixing Bottle at 2-8 °C for up to one month.
- During the preparation of the standard curve, make certain to mix the higher concentration well before making the next dilution. Use a new tip with each dilution.
- The plate should be read immediately after the assay is finished. If, however, the plate cannot be read immediately, seal the plate, cover with aluminum foil or an opaque lid, and store the plate at 2-8 °C for up to 24 hours. Prior to reading, agitate the plate on the plate shaker at room temperature for 10 minutes. Delay in reading a plate may result in decreased sensitivity for some analytes.
- The titer plate shaker should be set at a speed to provide maximum orbital mixing without splashing of liquid outside the wells. For the recommended plate shaker, this would be a setting of 5-7 which is approximately 500-800 rpm.
- Ensure that the needle probe is clean. This may be achieved by sonication and/or alcohol flushes.

- When reading the assay on the Luminex® 200™ instrument, adjust probe height according to the protocols recommended by Luminex® to the kit solid plate or to the recommended filter plates using 3 alignment discs. When reading the assay on the MAGPIX® instrument, adjust probe height according to the protocols recommended by Luminex®. When reading the assay on the FLEXMAP 3D® instrument, adjust probe height according to the protocols recommended by Luminex® to the kit solid plate using 1 alignment disc.
- For FLEXMAP 3D® when using the solid plate in the kit, the final resuspension should be with 150 µL Sheath Fluid PLUS in each well and 75 µL should be aspirated.
- For the xMAP® INTELLIFLEX instrument, adjust probe height based on the type of plate you are using, place an alignment disk or an alignment sphere in the well according to the protocol recommended by Luminex®.
- For cell culture supernatants or tissue extraction, use the culture or extraction medium as the matrix solution in background, standard curve and control wells. If samples are diluted in Assay Buffer, use the Assay Buffer as matrix.
- For serum/plasma samples that require further dilution beyond "Neat", use the Serum Matrix provided in the kit.
- For cell/tissue homogenate, the final cell or tissue homogenate should be prepared in a buffer that has a neutral pH, contains minimal detergents or strong denaturing detergents, and has an ionic strength close to physiological concentration. Avoid debris, lipids, and cell/tissue aggregates. Centrifuge samples before use.
- Vortex all reagents well before adding to plate.

Note: RANTES is provided as a separate bead vial in both premixed bead kits due to different dilution requirements for serum/plasma samples. RANTES can only be added in the premix for samples other than serum/plasma. If measuring RANTES in serum/plasma, it is recommended to use a singleplex kit including RANTES only. For more information, please carefully review the sample preparation for serum and plasma samples and the preparation of antibody-immobilized beads sections below when assaying RANTES.

Sample Collection and Storage

Preparation of Serum Samples

- Allow the blood to clot for at least 30 minutes before centrifugation for 10 minutes at 1000 x g. Remove serum and assay immediately or aliquot and store samples at $\leq -20^{\circ}\text{C}$.
- Avoid multiple (> 2) freeze/thaw cycles.
- When using frozen samples, it is recommended to thaw the samples completely, mix well by vortexing and centrifuge prior to use in the assay to remove particulates.
- Neat Serum samples (for measuring 47 analytes, not including RANTES) are used. When further dilution is required, use Serum Matrix as the diluent.
- When measuring RANTES in serum, samples should be diluted 1:100 in the Assay Buffer and a standard curve with Assay Buffer matrix should be used accordingly. When further dilution beyond 1:100 is required, use Assay Buffer as the diluent.

Preparation of Plasma Samples

- Plasma collection using EDTA as an anti-coagulant is recommended. Centrifuge for 10 minutes at 1000 x g within 30 minutes of blood collection. Remove plasma and assay immediately or aliquot and store samples at $\leq -20^{\circ}\text{C}$.
- Avoid multiple (> 2) freeze/thaw cycles.
- When using frozen samples, it is recommended to thaw the samples completely, mix well by vortexing and centrifuge prior to use in the assay to remove particulates.
- Neat Plasma samples (for measuring 47 analytes, not including RANTES) are used. When further dilution is required, use Serum Matrix as the diluent.
- When measuring RANTES in plasma, samples should be diluted 1:100 in the Assay Buffer and a standard curve with Assay Buffer matrix should be used accordingly. When further dilution beyond 1:100 is required, use Assay Buffer as the diluent.

Preparation of Tissue Culture Supernatant

- Centrifuge the sample to remove debris and assay immediately or aliquot and store samples at $\leq -20^{\circ}\text{C}$.
- Avoid multiple (> 2) freeze/thaw cycles.
- Tissue culture supernatant may require a dilution with an appropriate control medium prior to assay. Tissue/cell extracts should be done in neutral buffers containing reagents and conditions that do not interfere with assay performance. Excess concentrations of detergent, salt, denaturants, high or low pH, etc. will negatively affect the assay. Organic solvents should be avoided. The tissue/cell extract samples should be free of particles such as cells or tissue debris.

NOTE:

- A maximum of 25 μL per well of diluted or neat sample can be used.
- All samples must be stored in polypropylene tubes. **DO NOT STORE SAMPLES IN GLASS.**
- Avoid debris, lipids and cells when using samples with gross hemolysis or lipemia.
- Care must be taken when using heparin as an anti-coagulant since an excess of heparin will provide falsely high values. Use no more than 10 IU heparin per mL of blood collected.

Preparation of Reagents for Immunoassay

Preparation of Antibody-Immobilized Beads

If premixed beads are used, sonicate the premixed bead bottle 30 seconds in an ultrasonic water bath and then vortex for 1 minute before use.

To prepare a 38-Plex premixed beads or a 48-Plex premixed beads, which includes RANTES, add 70 μ L of RANTES beads to the 37-Plex premixed bead bottle or the 47-Plex premixed bead bottle, respectively.

Note: Due to high concentration of RANTES in serum/plasma, it has to be measured separately with 1:100 diluted serum/plasma. The 37-Plex premixed beads and the 47-Plex premixed beads are used for measuring all other 37 or 47 analytes, respectively, in serum/plasma with **Neat** serum/plasma. RANTES should only be added to the premix if running samples other than serum/plasma.

For individual vials of beads, sonicate each antibody-bead vial for 30 seconds in an ultrasonic water bath; vortex for 1 minute. Add 60 μ L from each antibody-bead vial to the Mixing Bottle and bring final volume to 3.0 mL with Bead Diluent. Vortex the mixed beads well. Unused portion may be stored at 2-8 °C for up to one month. (**Note:** Due to the composition of magnetic beads, you may notice a slight color in the bead solution. This does not affect the performance of the beads or the kit.)

Example 1: When using 20 antibody-immobilized beads, add 60 μ L from each of the 20 bead vials to the Mixing Bottle. Then add 1.8 mL Bead Diluent.

Example 2: When using 9 antibody-immobilized beads, add 60 μ L from each of the 9 bead vials to the Mixing Bottle. Then add 2.46 mL Bead Diluent.

Preparation of Quality Controls

Before use, reconstitute Quality Control 1 and Quality Control 2 with 250 μ L deionized water. Invert the vial several times to mix and vortex. Allow the vial to sit for 5-10 minutes. Transfer the reconstituted Quality Control 1 and Quality Control 2 into two polypropylene microfuge tubes and set in an ice bath. These should be added to the plate within 1 hour of reconstitution. Unused portion may be stored at $\leq -20^{\circ}\text{C}$ for up to one month.

Preparation of Wash Buffer

Bring the 10X Wash Buffer to room temperature and mix to bring all salts into solution. Dilute 60 mL of 10X Wash Buffer with 540 mL deionized water. Store the unused portion at 2-8 $^{\circ}\text{C}$ for up to one month.

Preparation of Serum Matrix

This step is required for serum or plasma samples only.

Add 1.0 mL deionized water to the bottle containing lyophilized Serum Matrix. Mix well. Allow at least 10 minutes for complete reconstitution. Leftover reconstituted Serum Matrix should be stored at $\leq -20^{\circ}\text{C}$ for up to one month.

Preparation of Human Cytokine/Chemokine/Growth Factor Panel A Standard

1. Prior to use, reconstitute the Human Cytokine/Chemokine/Growth Factor Panel A Standard with 250 μ L deionized water. Refer to table below for analyte concentrations. Invert the vial several times to mix. Vortex the vial for 10 seconds. Allow the vial to sit for 5-10 minutes. Transfer the reconstituted standard into a polypropylene microfuge tube. This will be used as Standard 7; This reconstituted standard and the serially diluted standards in the following steps should be set in an ice bath, during the assay procedure. These need to be added to the plate within 1 hour of preparation. The unused portion of the "Standard 7" may be stored at $\leq -20^{\circ}\text{C}$ for up to one month.


2. Preparation of Working Standards

Label 6 polypropylene microfuge tubes Standard 1 through Standard 6. Add 150 μL of Assay Buffer to each of the 6 tubes. Prepare serial dilutions by adding 50 μL of the reconstituted standard to the Standard 6 tube, mix well and transfer 50 μL of Standard 6 to the Standard 5 tube, mix well and transfer 50 μL of Standard 5 to the Standard 4 tube, mix well and transfer 50 μL of Standard 4 to the Standard 3 tube, mix well and transfer 50 μL of Standard 3 to the Standard 2 tube, mix well and transfer 50 μL of Standard 2 to the Standard 1 tube and mix well. The 0 pg/mL standard (Background) will be Assay Buffer.

Standard No.	Add Deionized Water (μL)	Add Standard (volume)
Standard 7	250	0

Standard No.	Add Assay Buffer (μL)	Add Standard (volume)
Standard 6	150	50 μL of Standard 7
Standard 5	150	50 μL of Standard 6
Standard 4	150	50 μL of Standard 5
Standard 3	150	50 μL of Standard 4
Standard 2	150	50 μL of Standard 3
Standard 1	150	50 μL of Standard 2

Preparation of Standards

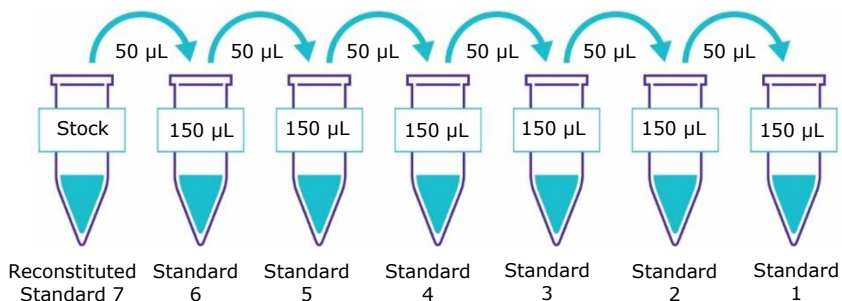

Standard	IL-9 (pg/mL)	IL-7, IL-18 (pg/mL)	FLT-3L (pg/mL)	IL-1RA (pg/mL)
Standard 1	0.61	0.98	1.1	1.2
Standard 2	2.4	3.9	4.4	4.8
Standard 3	9.7	16	18	19
Standard 4	39	63	70	77
Standard 5	156	250	281	306
Standard 6	625	1,000	1,125	1,225
Standard 7	2,500	4,000	4,500	4,900

Standard	IL-3, IL-4, IL-5, IL-17A (pg/mL)	MDC (pg/mL)	MIP-1β, GROα (pg/mL)	TNFβ (pg/mL)
Standard 1	1.2	1.3	1.5	1.6
Standard 2	4.9	5.4	5.9	6.3
Standard 3	20	21	23	25
Standard 4	78	86	94	102
Standard 5	313	344	375	406
Standard 6	1,250	1,375	1,500	1,625
Standard 7	5,000	5,500	6,000	6,500

Standard	IL-2, IL-15 (pg/mL)	IL-6, RANTES (pg/mL)	IFNγ, IL-8, IL-10, IL-12 (p70), TGFα (pg/mL)	IP-10 (pg/mL)
Standard 1	1.7	2.0	2.4	2.9
Standard 2	6.8	7.8	9.8	12
Standard 3	27	31	39	47
Standard 4	109	125	156	188
Standard 5	438	500	625	750
Standard 6	1,750	2,000	2,500	3,000
Standard 7	7,000	8,000	10,000	12,000

Standard	EGF, MCP-1, MIP-1α, VEGF-A (pg/mL)	TNFα (pg/mL)	Eotaxin (pg/mL)	IL-1β, IL-12 (p40), IL-13 (pg/mL)
Standard 1	3.7	4.9	5.1	6.1
Standard 2	15	19	21	24
Standard 3	59	78	82	98
Standard 4	234	312	328	391
Standard 5	937	1,250	1,313	1,563
Standard 6	3,730	5,000	5,250	6,250
Standard 7	15,000	20,000	21,000	25,000

Standard	G-CSF (pg/mL)	IFNα2, MCP-3, IL-1α (pg/mL)	GM-CSF (pg/mL)	PDGF-AA (pg/mL)
Standard 1	7.3	8.5	9.8	13
Standard 2	29	34	39	54
Standard 3	117	137	156	215
Standard 4	469	547	625	859
Standard 5	1,875	2,188	2,500	3,438
Standard 6	7,500	8,750	10,000	13,750
Standard 7	30,000	35,000	40,000	55,000

Standard	sCD40L (pg/mL)	IL-27 (pg/mL)	IL-17F, MIG (pg/mL)	Fractalkine (pg/mL)
Standard 1	20	22	24	26
Standard 2	78	88	98	103
Standard 3	313	352	391	410
Standard 4	1,250	1,406	1,563	1,641
Standard 5	5,000	5,625	6,250	6,563
Standard 6	20,000	22,500	25,000	26,250
Standard 7	80,000	90,000	100,000	105,000

Standard	FGF-2 (pg/mL)	M-CSF, PDGF-AB/BB (pg/mL)	IL-22 (pg/mL)	IL-17E (pg/mL)
Standard 1	29	37	44	68
Standard 2	115	146	176	273
Standard 3	459	586	703	1,094
Standard 4	1,836	2,344	2,813	4,375
Standard 5	7,344	9,375	11,250	17,500
Standard 6	29,375	37,500	45,000	70,000
Standard 7	117,500	150,000	180,000	280,000

Immunoassay Procedure

- Prior to beginning this assay, it is imperative to read this protocol completely and to thoroughly understand the Technical Guidelines.
- Allow all reagents to warm to room temperature (20-25 °C) before use in the assay.
- Diagram the placement of Standards 0 (Background), Standard 1 through 7, Controls 1 and 2, and Samples on Well Map Worksheet in a vertical configuration.

(Note: Most instruments will only read the 96-well plate vertically by default.) It is recommended to run the assay in duplicate.

1. Add 200 μ L of Wash Buffer into each well of the plate. Seal and mix on a plate shaker for 10 minutes at room temperature (20-25 °C).
2. Decant Wash Buffer and remove the residual amount from all wells by inverting the plate and tapping it smartly onto absorbent towels several times.
3. Add 25 μ L of each Standard or Control into the appropriate wells. Assay Buffer should be used for 0 pg/mL standard (Background).
4. Add 25 μ L of Assay Buffer to the sample wells.
5. Add 25 μ L of appropriate matrix solution to the background, standards, and control wells. When assaying serum or plasma, use the Serum Matrix provided in the kit. When assaying tissue culture or other supernatant, use proper control culture medium as the matrix solution. When measuring RANTES in serum or plasma use Assay Buffer as the matrix solution.
6. Add 25 μ L of Sample (1:100 dilution for RANTES if using serum or plasma samples, neat for all other analytes) into the appropriate wells.
7. Vortex Mixing Bottle and add 25 μ L of the Mixed or Premixed Beads to each well. **(Note:** During addition of Beads, shake bead bottle intermittently to avoid settling.)
8. Seal the plate with a plate sealer. Wrap the plate with foil and incubate with agitation on a plate shaker overnight (16-18 hours) at 2-8 °C. Alternatively, incubate for 2 hours at room temperature (20-25 °C).

Add 200 μ L Wash Buffer per well



Shake 10 min, RT
Decant

- Add 25 μ L Standard or Control to appropriate wells
- Add 25 μ L Assay Buffer to background and sample wells
- Add 25 μ L appropriate matrix solution to background, standards, and control wells
- Add 25 μ L Samples to sample wells
- Add 25 μ L Beads to each well



Incubate overnight (16-18 hours) at 2-8 °C or 2 hours at RT with shaking

9. Gently remove well contents and wash plate 3 times following instructions listed in the Plate Washing section.
10. Add 25 μ L of Detection Antibodies into each well.
(**Note:** Allow the Detection Antibodies to warm to room temperature prior to addition.)
11. Seal, cover with foil and incubate with agitation on a plate shaker for 1 hour at room temperature (20-25 $^{\circ}$ C). **DO NOT ASPIRATE AFTER INCUBATION.**
12. Add 25 μ L Streptavidin-Phycoerythrin to each well containing the 25 μ L of Detection Antibodies.
13. Seal, cover with foil and incubate with agitation on a plate shaker for 30 minutes at room temperature (20-25 $^{\circ}$ C).
14. Gently remove well contents and wash plate 3 times following instructions listed in the Plate Washing section.
15. Add 150 μ L of Sheath Fluid PLUS (or Drive Fluid PLUS if using MAGPIX[®]) to all wells. Resuspend the beads on a plate shaker for 5 minutes.
16. Run plate on Luminex[®] 200[™], HTS, FLEXMAP 3D[®], MAGPIX[®] instrument with xPONENT[®] software or xMAP[®] INTELLIFLEX instrument with INTELLIFLEX software.
17. Save and analyze the Median Fluorescent Intensity (MFI) data using a 5-parameter logistic or spline curve-fitting method for calculating analyte concentrations in samples.
(**Note:** For diluted samples, multiply the calculated concentration by the dilution factor.)



Remove well contents and wash 3X with 200 μ L Wash Buffer

Add 25 μ L Detection Antibodies per well



Incubate 1 hour at RT

Do Not Aspirate

Add 25 μ L Streptavidin-Phycoerythrin per well



Incubate for 30 minutes at RT

Remove well contents and wash 3X with 200 μ L Wash Buffer

Add 150 μ L Sheath Fluid PLUS or Drive Fluid per well

Read on Luminex[®] (100 μ L, 50 beads per bead set)

Plate Washing

If using a solid plate, use either a handheld magnet or magnetic plate washer.

- Handheld magnet (Cat. No. 40-285)
Rest plate on magnet for 60 seconds to allow complete settling of magnetic beads. Remove well contents by gently decanting the plate in an appropriate waste receptacle and gently tapping on absorbent pads to remove residual liquid. Wash plate with 200 μ L of Wash Buffer by removing plate from magnet, adding Wash Buffer, shaking for 30 seconds, reattaching to magnet, letting beads settle for 60 seconds and removing well contents as previously described after each wash. Repeat wash steps as recommended in Assay Procedure.
- Magnetic plate washer (Cat. No. 40-094, 40-095, 40-096 and 40-097)
Please refer to specific automatic plate washer manual for appropriate equipment settings. Please note that after the final aspiration, there will be approximately 25 μ L of residual wash buffer in each well. This is expected when using the BioTek[®] plate washer and this volume does not need to be aspirated from the plate.

Equipment Settings

Luminex[®] 200™, HTS, FLEXMAP 3D[®], MAGPIX[®] instruments with xPONENT[®] software and xMAP[®] INTELLIFLEX instrument with INTELLIFLEX software:

These specifications are for the above listed instruments and software. Luminex[®] instruments with other software (for example, MasterPlex[®], StarStation, LiquiChip, Bio-Plex[®] Manager™, LABScan™100) would need to follow instrument instructions for gate settings and additional specifications from the vendors for reading Luminex[®] magnetic beads.

For magnetic bead assays, each instrument must be calibrated and performance verified with the indicated calibration and verification kits.

Instrument	Calibration Kit	Verification Kit
Luminex® 200™ and HTS	xPONENT® 3.1 compatible Calibration Kit (Cat. No. LX2RCAL-K25)	Performance Verification Kit (Cat. No. LX2RPVER-K25)
FLEXMAP 3D®	FLEXMAP 3D® Calibrator Kit (Cat. No. F3DCAL-K25)	FLEXMAP 3D® Performance Verification Kit (Cat. No. F3DPVER-K25)
xMAP® INTELLIFLEX	xMAP® INTELLIFLEX Calibration Kit (Cat. No. IFX-CAL-K20)	xMAP® INTELLIFLEX Performance Verification Kit (Cat. No. IFX-PVER-K20)
MAGPIX®	MAGPIX® Calibration Kit (Cat. No. MPXCAL-K25)	MAGPIX® Performance Verification Kit (Cat. No. MPXPVER-K25)

NOTE: When setting up a Protocol using the xPONENT® software, you must select MagPlex® as the Bead Type in the Acquisition settings.

NOTE: These assays cannot be run on any instruments using Luminex® IS 2.3 or Luminex® 1.7 software.

The Luminex® probe height must be adjusted to the plate provided in the kit. Please use Cat. No. MAG-PLATE, if additional plates are required for this purpose.

Events	50, per bead		
Sample Size	100 µL		
Gate Settings	8,000 to 15,000		
Reporter Gain	Default (low PMT)		
Time Out	60 seconds		
Bead Set	Customizable 48-plex Beads		
sCD40L	12	IL-12 (p70)	44
EGF	13	IL-13	46
Eotaxin	14	IL-15	47
FGF-2	15	IL-17A	48
FLT-3L	18	IL-17E/IL-25	51
Fractalkine	19	IL-17F	53
G-CSF	20	IL-18	54
GM-CSF	21	IL-22	55
GRO α	22	IL-27	56
IFN α 2	25	IP-10	57
IFN γ	26	MCP-1	61
IL-1 α	27	MCP-3	62
IL-1 β	28	M-CSF	63
IL-1RA	29	MDC	64
IL-2	30	MIG	65
IL-3	33	MIP-1 α	66
IL-4	34	MIP-1 β	67
IL-5	35	PDGF-AA	72
IL-6	36	PDGF-AB/BB	73
IL-7	37	RANTES	74
IL-8	38	TGF α	75
IL-9	39	TNF α	76
IL-10	42	TNF β	77
IL-12 (p40)	43	VEGF-A	78

Quality Controls

The ranges for each analyte in Quality Control 1 and 2 are provided on the card insert or can be located at our website SigmaAldrich.com using the catalogue number as the keyword.

Assay Characteristics

Cross-Reactivity

There was no or negligible cross-reactivity between the antibodies for an analyte and any of the other analytes in this panel, except IL-12 (p40) had ~8% cross-reactivity with IL-12 (p70).

Assay Sensitivities (minimum detectable concentrations, pg/mL)

Minimum Detectable Concentration (MinDC) is calculated using MILLIPLEX® Analyst 5.1. It measures the true limits of detection for an assay by mathematically determining what the empirical MinDC would be if an infinite number of standard concentrations were run for the assay under the same conditions.

Analyte	Overnight Protocol (n = 3 Assays)		2 Hour Protocol (n = 3 Assays)	
	MinDC (pg/mL)	MinDC+2SD (pg/mL)	MinDC (pg/mL)	MinDC+2SD (pg/mL)
sCD40L	14.93	27.54	19.73	45.58
EGF	3.38	4.66	2.62	4.39
Eotaxin	2.97	3.11	2.19	2.80
FGF-2	27.67	29.13	28.02	39.57
FLT-3L	0.42	0.75	0.72	1.54
Fractalkine	7.87	13.42	9.09	15.72
G-CSF	3.66	6.35	3.12	8.43
GM-CSF	8.47	8.86	4.42	10.85
GRO α	1.05	1.49	0.41	0.49
IFN α 2	6.79	10.84	1.97	2.21
IFN γ	1.88	2.13	1.84	2.84
IL-1 α	5.32	7.43	3.24	6.62
IL-1 β	2.73	5.53	1.14	1.55
IL-1RA	0.30	0.47	0.54	1.13
IL-2	0.62	0.97	0.44	0.73
IL-3	0.35	0.60	0.50	0.95
IL-4	0.34	0.79	0.31	0.53
IL-5	0.22	0.24	0.34	0.35
IL-6	0.43	0.60	0.56	1.06
IL-7	0.25	0.38	0.29	0.63
IL-8	2.01	2.64	0.95	1.85

For research use only. Not for use in diagnostic procedures.

Analyte	Overnight Protocol (n = 3 Assays)		2 Hour Protocol (n = 3 Assays)	
	MinDC (pg/mL)	MinDC+2SD (pg/mL)	MinDC (pg/mL)	MinDC+2SD (pg/mL)
IL-9	5.01	6.59	11.36	21.04
IL-10	0.78	1.35	0.87	1.61
IL-12 (p40)	2.91	6.31	4.38	7.27
IL-12 (p70)	0.87	1.36	1.91	2.06
IL-13	2.24	5.56	1.40	1.58
IL-15	0.41	0.52	0.58	1.05
IL-17A	0.59	1.21	1.56	2.19
IL-17E/IL-25	41.30	80.52	16.69	25.85
IL-17F	6.10	7.35	7.52	12.80
IL-18	0.68	1.58	0.58	1.08
IL-22	30.09	53.10	41.15	44.63
IL-27	17.89	26.29	15.60	37.16
IP-10	2.66	3.07	3.26	4.62
MCP-1	3.02	3.78	1.07	1.55
MCP-3	10.47	11.69	6.48	13.26
M-CSF	9.38	15.43	10.60	18.27
MDC	0.84	1.45	0.43	0.80
MIG	7.62	12.35	12.65	25.89
MIP-1 α	3.98	4.90	2.40	5.39
MIP-1 β	1.24	1.84	4.15	7.20
PDGF-AA	7.13	17.24	5.14	9.90
PDGF-AB/BB	47.16	81.38	23.19	38.78
RANTES	1.79	1.83	0.67	0.92
TGF α	1.25	2.97	0.87	1.60
TNF α	1.57	3.30	0.98	1.52
TNF β	0.62	0.81	1.43	2.11
VEGF-A	1.46	3.30	2.38	4.15

Precision

Intra-assay precision is generated from the mean of the %CV's from 8 reportable results across two different concentrations of analytes in a single assay. Inter-assay precision is generated from the mean of the %CV's across two different concentrations of analytes across 6 different assays.

Analyte	Overnight Protocol		2 Hour Protocol
	Intra-assay %CV	Inter-assay %CV	Intra-assay %CV
sCD40L	< 15%	< 20%	< 15%
EGF	< 15%	< 20%	< 15%
Eotaxin	< 15%	< 20%	< 15%
FGF-2	< 15%	< 20%	< 15%
FLT-3L	< 15%	< 20%	< 15%
Fractalkine	< 15%	< 20%	< 15%
G-CSF	< 15%	< 20%	< 15%
GM-CSF	< 15%	< 20%	< 15%
GRO α	< 15%	< 20%	< 15%
IFN α 2	< 15%	< 20%	< 15%
IFN γ	< 15%	< 25%	< 15%
IL-1 α	< 15%	< 20%	< 15%
IL-1 β	< 15%	< 20%	< 15%
IL-1RA	< 15%	< 20%	< 15%
IL-2	< 15%	< 20%	< 15%
IL-3	< 15%	< 20%	< 15%
IL-4	< 15%	< 20%	< 15%
IL-5	< 15%	< 20%	< 15%
IL-6	< 15%	< 20%	< 15%
IL-7	< 15%	< 20%	< 15%
IL-8	< 15%	< 20%	< 15%
IL-9	< 15%	< 20%	< 15%
IL-10	< 15%	< 20%	< 15%
IL-12 (p40)	< 15%	< 20%	< 15%
IL-12 (p70)	< 15%	< 20%	< 15%

For research use only. Not for use in diagnostic procedures.

Analyte	Overnight Protocol		2 Hour Protocol
	Intra-assay %CV	Inter-assay %CV	Intra-assay %CV
IL-13	< 15%	< 20%	< 15%
IL-15	< 15%	< 20%	< 15%
IL-17A	< 15%	< 20%	< 15%
IL-17E/IL-25	< 15%	< 20%	< 15%
IL-17F	< 15%	< 20%	< 15%
IL-18	< 15%	< 20%	< 15%
IL-22	< 15%	< 20%	< 15%
IL-27	< 15%	< 20%	< 15%
IP-10	< 15%	< 20%	< 15%
MCP-1	< 15%	< 20%	< 15%
MCP-3	< 15%	< 20%	< 15%
M-CSF	< 15%	< 20%	< 15%
MDC	< 15%	< 20%	< 15%
MIG	< 15%	< 20%	< 15%
MIP-1 α	< 15%	< 20%	< 15%
MIP-1 β	< 15%	< 20%	< 15%
PDGF-AA	< 15%	< 20%	< 15%
PDGF-AB/BB	< 15%	< 20%	< 15%
RANTES	< 15%	< 20%	< 15%
TGF	< 15%	< 20%	< 15%
TNF α	< 15%	< 20%	< 15%
TNF β	< 15%	< 20%	< 15%
VEGF-A	< 15%	< 20%	< 15%

Accuracy

Spike Recovery: The data represent mean percent recovery of spiked standards ranging from low, medium, and high concentration in serum matrices (n=6).

Overnight Protocol		Overnight Protocol	
Analyte	% Recovery in Serum Matrix	Analyte	% Recovery in Serum Matrix
sCD40L	95	IL-12 (p70)	96
EGF	101	IL-13	95
Eotaxin	96	IL-15	96
FGF-2	106	IL-17A	93
FLT-3L	95	IL-17E/IL-25	93
Fractalkine	98	IL-17F	95
G-CSF	97	IL-18	97
GM-CSF	100	IL-22	96
GRO α	99	IL-27	96
IFN α 2	98	IP-10	99
IFN γ	94	MCP-1	101
IL-1 α	98	MCP-3	104
IL-1 β	92	M-CSF	97
IL-1RA	97	MDC	96
IL-2	95	MIG	95
IL-3	100	MIP-1 α	104
IL-4	95	MIP-1 β	99
IL-5	99	PDGF-AA	102
IL-6	96	PDGF-AB/BB	91
IL-7	97	RANTES	93
IL-8	96	TGF α	102
IL-9	101	TNF α	101
IL-10	98	TNF β	99
IL-12 (p40)	95	VEGF-A	99

For research use only. Not for use in diagnostic procedures.

Troubleshooting

Problem	Probable Cause	Solution
Insufficient bead count	Plate washer aspirate height set too low	Adjust aspiration height according to manufacturers' instructions.
	Bead mix prepared inappropriately	Sonicate bead vials in an ultrasonic waterbath and vortex just prior to adding to bead mix bottle according to protocol. Agitate bead mix intermittently in reservoir while pipetting this into the plate.
	Samples cause interference due to particulate matter or viscosity	See above. Also sample probe may need to be cleaned with alcohol flushes, back flushes and washes; or if needed, probe should be removed and sonicated.
	Probe height not adjusted correctly	When reading the assay on the Luminex® 200™ instrument, adjust probe height to the kit solid plate using 3 alignment discs. When reading the assay on the MAGPIX® instrument, adjust probe height to the kit solid plate using 2 alignment discs. When reading the assay on the FLEXMAP 3D® instrument, adjust probe height to the kit solid plate using 1 alignment disc. When reading the assay on the xMAP® INTELLIFLEX instrument, adjust probe height based on the type of plate you are using, place an alignment disk or an alignment sphere in the well according to the protocol recommended by Luminex®."
Background is too high	Background wells were contaminated	Avoid cross-well contamination by using sealer appropriately and pipetting with multichannel pipettes without touching reagent in plate.
	Matrix used has endogenous analyte or interference	Check matrix ingredients for cross-reacting components (for example, interleukin modified tissue culture medium).
	Insufficient washes	Increase number of washes.

Problem	Probable Cause	Solution
Beads not in region or gate	Luminex® instrument not calibrated correctly or recently	Calibrate Luminex® instrument based on manufacturer's instructions, at least once a week or if temperature has changed by > 3 °C.
	Gate settings not adjusted correctly	Some Luminex® instruments (for example, Bio-Plex®) require different gate settings than those described in the kit protocol. Use instrument default settings.
	Wrong bead regions in protocol template	Check kit protocol for correct bead regions or analyte selection.
	Incorrect sample type used	Samples containing organic solvents or if highly viscous should be diluted or dialyzed as required.
	Instrument not washed or primed	Prime the Luminex® instrument 4 times to rid it of air bubbles, wash 4 times with sheath fluid or water if there is any remnant alcohol or sanitizing liquid.
	Beads were exposed to light	Keep plate and bead mix covered with dark lid or aluminum foil during all incubation steps.
Signal for whole plate is same as background	Incorrect or no Detection Antibody was added	Add appropriate Detection Antibody and continue.
	Streptavidin-Phycoerythrin was not added	Add Streptavidin-Phycoerythrin according to protocol. If Detection Antibody has already been removed, sensitivity may be low.
Low signal for standard curve	Detection Antibody may have been removed prior to adding Streptavidin-Phycoerythrin	May need to repeat assay if desired sensitivity not achieved.
	Incubations done at inappropriate temperatures, timings or agitation	Assay conditions need to be checked.

Problem	Probable Cause	Solution
Signals too high, standard curves are saturated	Calibration target value set too high	With some Luminex® instruments (for example, Bio-Plex®) default target setting for RP1 calibrator is set at high PMT. Use low target value for calibration and reanalyze plate.
	Plate incubation was too long with standard curve and samples	Use shorter incubation time.
Sample readings are out of range	Samples contain no or below detectable levels of analyte	If below detectable levels, it may be possible to use higher sample volume. Check with technical support for appropriate protocol modifications.
	Samples contain analyte concentrations higher than highest standard point	Samples may require dilution and reanalysis for just that particular analyte.
	Standard curve was saturated at higher end of curve	See above.
High variation in samples and/or standards	Multichannel pipette may not be calibrated	Calibrate pipettes.
	Plate washing was not uniform	Confirm all reagents are removed completely in all wash steps.
	Samples may have high particulate matter or other interfering substances	See above.
	Plate agitation was insufficient	Plate should be agitated during all incubation steps using an orbital plate shaker at a speed where beads are in constant motion without causing splashing.
	Cross-well contamination	Check when reusing plate sealer that no reagent has touched sealer. Care should be taken when using same pipette tips that are used for reagent additions and that pipette tip does not touch reagent in plate.

***Note:** If using a filter plate, contact Technical Support with any questions.

Product Ordering

Replacement Reagents

Reagent	Note	Cat. No.
Human Cytokine Panel A Standard 1	For configurable kit	HCYTA-8060-1
Human Cytokine Panel A Standard 2	For 38- or 48-Plex or configurable kit	HCYTA-8060-2
Human Panel A Quality Controls 1 and 2 for Standard 1	For configurable kit	HCYTA-6060-1
Human Cytokine Panel A Quality Controls 1 and 2 for Standard 2	For 38- or 48-Plex or configurable kit	HCYTA-6060-2
Human Cytokine Panel A Serum Matrix		MXHSM-A
Human Cytokine Panel A Detection Antibodies 1	For configurable kit	HCYTA-1060-1
Human Cytokine Panel A Detection Antibodies 2	For 38- or 48-Plex or configurable kit	HCYTA-1060-2
Streptavidin-Phycoerythrin	For configurable kit	L-SAPE3
Streptavidin-Phycoerythrin	For 38- or 48-Plex or configurable kit	L-SAPE10
Assay Buffer		L-AB
Set of two 96-Well plates with sealers		MAG-PLATE
10X Wash Buffer		L-WB
Bead Diluent		LBD

For research use only. Not for use in diagnostic procedures.

Reagent	Note	Cat. No.
Premixed 37-Plex Beads*		HCYTAPX37-MG
Premixed 47-Plex Beads*		HCYTAPX47-MG
Human Cytokine/Chemokine/Growth Factor Panel A 38 Plex Premixed Magnetic Bead Panel		HCYTA-60K-PX38
Human Cytokine/Chemokine/Growth Factor Panel A 48 Plex Premixed Magnetic Bead Panel		HCYTA-60K-PX48
Human Cytokine/Chemokine/Growth Factor Panel A 38 Plex Premixed Magnetic Bead Panel – BULK PACKAGING		HCYTA-60K-PXBK38
Human Cytokine/Chemokine/Growth Factor Panel A 48 Plex Premixed Magnetic Bead Panel – BULK PACKAGING		HCYTA-60K-PXBK48
Human Cytokine Panel A + B 76-Plex Combo Pack		HCYTPAB-76SK
Human Cytokine/Chemokine/Growth Factor Panel A 38 Plex Premixed Magnetic Bead Panel (in Combo Pack)		HCYTPA-76K
Human Cytokine Panel A + B 96-Plex Combo Pack		HCYTPAB-96SK
Human Cytokine/Chemokine/Growth Factor Panel A 48 Plex Premixed Magnetic Bead Panel (in Combo Pack)		HCYTPA-96K

*** For individual beads, see below.**

Antibody-Immobilized Magnetic Beads

Analyte	Bead No.	Cat. No.	Analyte	Bead No.	Cat. No.
sCD40L	12	HCD40L-MG	IL-13	46	HIL13-MG
EGF	13	HEGF-MG	IL-15	47	HIL15-MG
Eotaxin	14	HETXN-MG	IL-17A	48	HIL17A-MG
FGF-2	15	HFGF2-MG	IL-17E/IL-25	51	HIL17E-MG
FLT-3L	18	HFLT3L-MG	IL-17F	53	HIL17F-MG
Fractalkine	19	HFRACTALKN-MG	IL-18	54	HIL18-MG
G-CSF	20	HGCSF-MG	IL-22	55	HIL22-MG
GM-CSF	21	HGMCSF-MG	IL-27	56	HIL27-MG
GRO α	22	HGR0-MG	IP-10	57	HIP10-MG
IFN α 2	25	HIFNA2-MG	MCP-1	61	HMCP1-MG
IFN γ	26	HIFNG-MG	MCP-3	62	HMCP3-MG
IL-1 α	27	HIL1A-MG	M-CSF	63	HMCSF-MG
IL-1 β	28	HIL1B-MG	MDC	64	HMDC-MG
IL-1RA	29	HIL1RA-MG	MIG	65	HMIG-MG
IL-2	30	HIL2-MG	MIP-1 α	66	HMIP1A-MG
IL-3	33	HIL3-MG	MIP-1 β	67	HMIP1B-MG
IL-4	34	HIL4-MG	PDGF-AA	72	HPDGF-AA-MG
IL-5	35	HIL5-MG	PDGF-AB/BB	73	HPDGFBB-MG
IL-6	36	HIL6-MG	RANTES	74	HRANTES-MG
IL-7	37	HIL7-MG	TGF α	75	HTGFA-MG
IL-8	38	HIL8-MG	TNF α	76	HTNFA-MG
IL-9	39	HIL9-MG	TNF β	77	HTNFB-MG
IL-10	42	HIL10-MG	VEGF-A	78	HVEGFA-MG
IL-12 (p40)	43	HIL12P40-MG	Premixed 37-Plex Beads	HCYTAPX37-MG	
IL-12 (p70)	44	HIL12P70-MG	Premixed 47-Plex Beads	HCYTAPX47-MG	

Analyte Contents of Select Reagents

Analyte/ Bead Name	Luminex® Magnetic Bead Region	Customizable 48 Analytes (50X concentration, 90 µL)		HCYTAPX37-MG (37-Plex Premixed Beads)	HCYTAPX47-MG (47-Plex Premixed Beads)	HCYT-A-8060-1 (27-Plex Standard Mix)	HCYT-A-8060-2 (48-Plex Standard Mix)	HCYT-A-1060-1 (27-Plex Detection Mix); with L-SAPE3	HCYT-A-1060-2 (48-Plex Detection Mix); with L-SAPE10
		Available	Cat. No.						
Anti-Human sCD40L	12	✓	HCD40L-MG		✓		✓		✓
Anti-Human EGF	13	✓	HEGF-MG	✓	✓		✓		✓
Anti-Human Eotaxin	14	✓	HETXN-MG	✓	✓		✓		✓
Anti-Human FGF-2	15	✓	HFGF2-MG		✓		✓		✓
Anti-Human FLT-3L	18	✓	HFLT3L-MG		✓		✓		✓
Anti-Human Fractalkine	19	✓	HFRACTALKN-MG		✓		✓		✓
Anti-Human G-CSF	20	✓	HGCSF-MG	✓	✓	✓	✓	✓	✓
Anti-Human GM-CSF	21	✓	HGMCSF-MG	✓	✓	✓	✓	✓	✓
Anti-Human GROα	22	✓	HGR0-MG		✓		✓		✓
Anti-Human IFNα2	25	✓	HIFNA2-MG	✓	✓		✓		✓
Anti-Human IFNγ	26	✓	HIFNG-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-1α	27	✓	HIL1A-MG	✓	✓		✓		✓
Anti-Human IL-1β	28	✓	HIL1B-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-1RA	29	✓	HIL1RA-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-2	30	✓	HIL2-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-3	33	✓	HIL3-MG	✓	✓		✓		✓

For research use only. Not for use in diagnostic procedures.

Analyte/ Bead Name	Luminex® Magnetic Bead Region	Customizable 48 Analytes (50X concentration, 90 µL)		HCYTAPX37-MG (37-Plex Premixed Beads)	HCYTAPX47-MG (47-Plex Premixed Beads)	HCYTA-8060-1 (27-Plex Standard Mix)	HCYTA-8060-2 (48-Plex Standard Mix)	HCYTA-1060-1 (27-Plex Detection Mix); with L-SAPE3	HCYTA-1060-2 (48-Plex Detection Mix); with L-SAPE10
		Available	Cat. No.						
Anti-Human IL-4	34	✓	HIL4-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-5	35	✓	HIL5-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-6	36	✓	HIL6-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-7	37	✓	HIL7-MG	✓	✓		✓		✓
Anti-Human IL-8	38	✓	HIL8-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-9	39	✓	HIL9-MG		✓		✓		✓
Anti-Human IL-10	42	✓	HIL10-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-12 (p40)	43	✓	HIL12P40-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-12 (p70)	44	✓	HIL12P70-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-13	46	✓	HIL13-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-15	47	✓	HIL15-MG	✓	✓		✓		✓
Anti-Human IL-17A	48	✓	HIL17A-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-17E/IL-25	51	✓	HIL17E-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-17F	53	✓	HIL17F-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-18	54	✓	HIL18-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-22	55	✓	HIL22-MG	✓	✓	✓	✓	✓	✓
Anti-Human IL-27	56	✓	HIL27-MG		✓	✓	✓	✓	✓

For research use only. Not for use in diagnostic procedures.

Analyte/ Bead Name	Luminex® Magnetic Bead Region	Customizable 48 Analytes (50X concentration, 90 µL)		HCYTAPX37-MG (37-Plex Premixed Beads)	HCYTAPX47-MG (47-Plex Premixed Beads)	HCYTA-8060-1 (27-Plex Standard Mix)	HCYTA-8060-2 (48-Plex Standard Mix)	HCYTA-1060-1 (27-Plex Detection Mix); with L-SAPE3	HCYTA-1060-2 (48-Plex Detection Mix); with L-SAPE10
		Available	Cat. No.						
Anti-Human IP-10	57	✓	HIP10-MG	✓	✓	✓	✓	✓	✓
Anti-Human MCP-1	61	✓	HMCP1-MG	✓	✓	✓	✓	✓	✓
Anti-Human MCP-3	62	✓	HMCP3-MG		✓		✓		✓
Anti-Human M-CSF	63	✓	HMCSF-MG	✓	✓	✓	✓	✓	✓
Anti-Human MDC	64	✓	HMDC-MG		✓		✓		✓
Anti-Human MIG/CXCL9	65	✓	HMIG-MG	✓	✓	✓	✓	✓	✓
Anti-Human MIP-1α	66	✓	HMIP1A-MG	✓	✓		✓		✓
Anti-Human MIP-1β	67	✓	HMIP1B-MG	✓	✓	✓	✓	✓	✓
Anti-Human PDGF-AA	72	✓	HPDGFAA-MG	✓	✓		✓		✓
Anti-Human PDGF-AB/BB	73	✓	HPDGFBB-MG	✓	✓		✓		✓
Anti-Human RANTES	74	✓	HRANTES-MG			✓	✓	✓	✓
Anti-Human TGFα	75	✓	HTGFA-MG		✓		✓		✓
Anti-Human TNFα	76	✓	HTNFA-MG	✓	✓	✓	✓	✓	✓
Anti-Human TNFβ	77	✓	HTNFB-MG	✓	✓		✓		✓
Anti-Human VEGF-A	78	✓	HVEGFA-MG	✓	✓		✓		✓

For research use only. Not for use in diagnostic procedures.

Well Map

	1	2	3	4	5	6	7	8	9	10	11	12
A	Standard 0 (Background)	Standard 4	QC-1 Control	Etc.								
B	Standard 0 (Background)	Standard 4	QC-1 Control									
C	Standard 1	Standard 5	QC-2 Control									
D	Standard 1	Standard 5	QC-2 Control									
E	Standard 2	Standard 6	Sample 1									
F	Standard 2	Standard 6	Sample 1									
G	Standard 3	Standard 7	Sample 2									
H	Standard 3	Standard 7	Sample 2									

Notice

We provide information and advice to our customers on application technologies and regulatory matters to the best of our knowledge and ability, but without obligation or liability. Existing laws and regulations are to be observed in all cases by our customers. This also applies in respect to any rights of third parties. Our information and advice do not relieve our customers of their own responsibility for checking the suitability of our products for the envisaged purpose.

The information in this document is subject to change without notice and should not be construed as a commitment by the manufacturing or selling entity, or an affiliate. We assume no responsibility for any errors that may appear in this document.

By purchasing this product, which contains fluorescently labeled microsphere beads authorized by Luminex® Corporation ("Luminex®"), you, the customer, acquire the right under the Luminex® patent rights, if any, to use this product or any portion of this product, including without limitation the microsphere beads contained herein, only with the Luminex® laser based fluorescent analytical test instrumentation marketed under the name of Luminex® 200™, HTS, FLEXMAP 3D®, xMAP® INTELLIFLEX, MAGPIX®.

Contact Information

For the location of the office nearest you, go to SigmaAldrich.com/offices.

Technical Assistance

Visit the tech service page at SigmaAldrich.com/techservice.

Standard Warranty

The applicable warranty for the products listed in this publication may be found at SigmaAldrich.com/terms.

Safety Data Sheets (SDS)

Safety Data Sheets are available on the product page at SigmaAldrich.com.

The life science business of Merck KGaA, Darmstadt, Germany operates as MilliporeSigma in the U.S. and Canada.

MilliporeSigma, Millipore, Milliplex and Sigma-Aldrich are trademarks of Merck KGaA, Darmstadt, Germany or its affiliates. All other trademarks are the property of their respective owners. Detailed information on trademarks is available via publicly accessible resources.

© 2019-2025 Merck KGaA, Darmstadt, Germany and/or its affiliates.
All Rights Reserved.
Template 00011187FM v. 20.0

For research use only. Not for use in diagnostic procedures.

20422338 Rev 09/25

**Millipore
Sigma**